


# Microbiome and metabolomics products

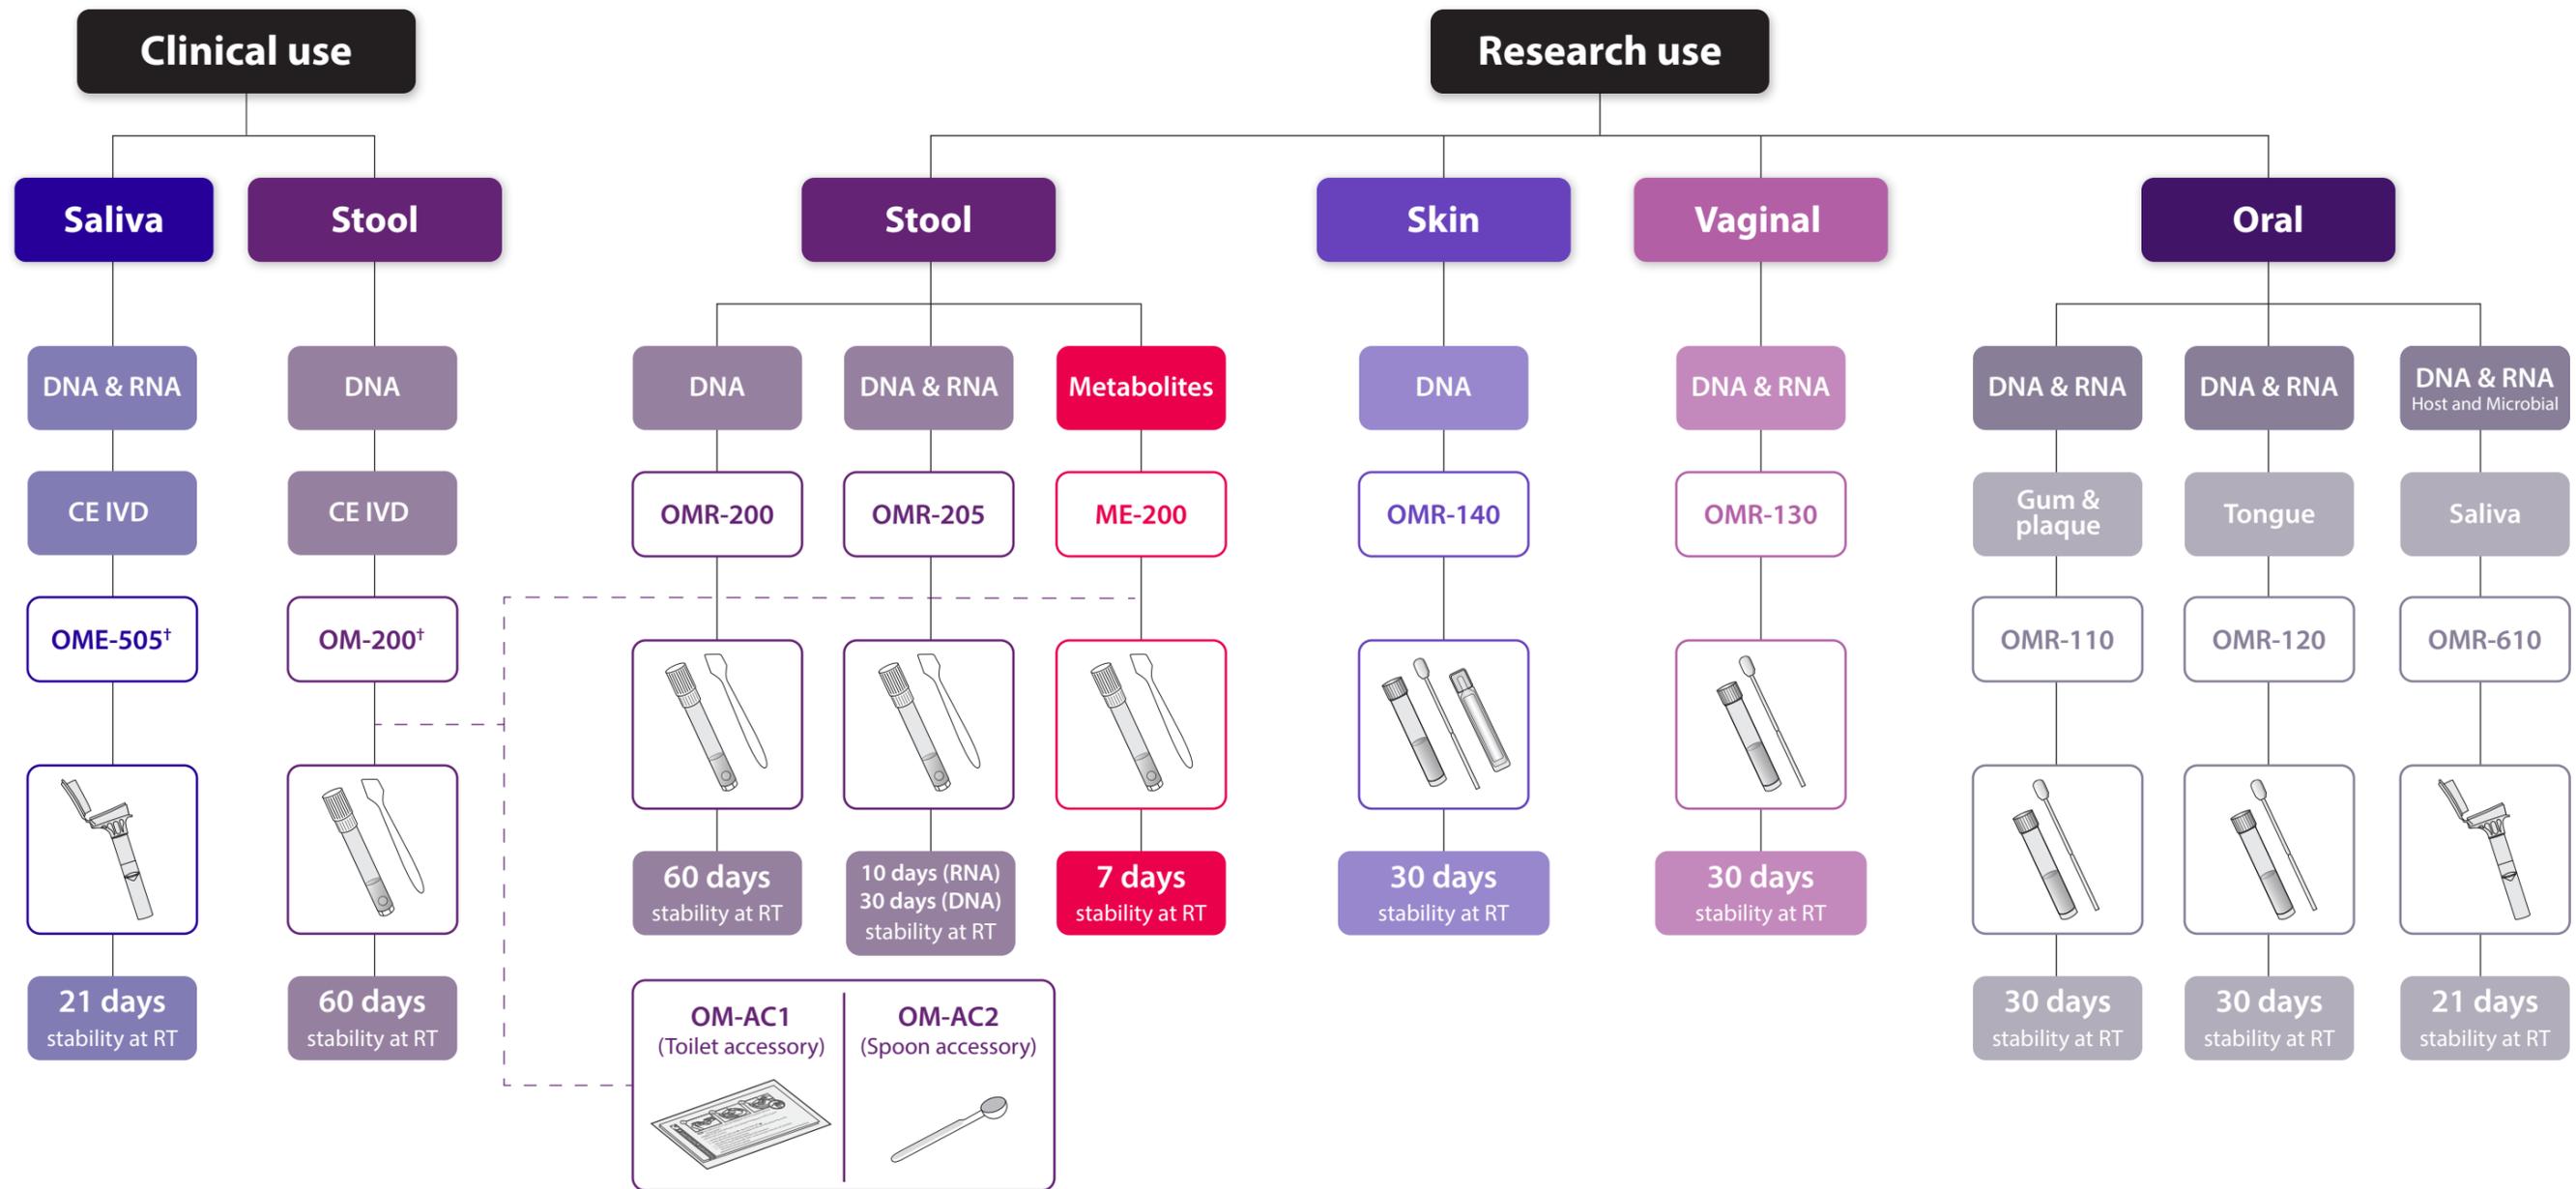

Some DNA Genotek products may not be available in all geographic regions.

† OMNIgene™•GUT (OM-200) and OMNIgene™•ORAL (OME-505) devices are CE marked for in vitro diagnostic use. The OMNIgene™•GUT (OM-200) device is not available for sale in the United States.

OMNIgene™•GUT (OMR-200), OMNIgene™•ORAL (OMR-110/120), OMNIgene™•VAGINAL, OMNIgene™•SALIVA (OMR-610) and OMNIgene™•SKIN devices are for research use only, not for use in diagnostic procedures.

OMNIgene, OMNImet and DNA Genotek are trademarks of DNA Genotek Inc.

Patent (www.dnagenotek.com/legalnotices)

© 2023 DNA Genotek Inc. is a subsidiary of OraSure Technologies, Inc., all rights reserved.


MK-01281 Issue 4/2023-12

Global market use  
(Outside U.S.)



Superior samples • Proven performance

[www.dnagenotek.com](http://www.dnagenotek.com)

	<b>Stool OM-200 (DNA)</b>	<b>Stool OMR-205 (DNA &amp; RNA)</b>	<b>Vaginal OMR-130 (DNA &amp; RNA)</b>	<b>Tongue OMR-120 (DNA &amp; RNA)</b>	<b>Gum &amp; plaque OMR-110 (DNA &amp; RNA)</b>	<b>Skin OMR-140 (DNA)</b>	<b>Saliva OME-505 (DNA &amp; RNA)</b>	<b>Saliva OMR-610 (DNA &amp; RNA Host and Microbial)</b>	<b>Stool ME-200 (Metabolites)</b>
									
Tare weight for collection device (weight of tube, cap, chemistry and swab, if applicable)	13.82 g	15.80 g	5.33 g	5.33 g	5.33 g	5.62 g	6.04 g	6.04 g	13.77 g
Volume of chemistry	2 mL	4 mL	1 mL	1 mL	1 mL	1 mL	1 mL	1 mL	2.8 mL
Volume of sample collected	0.4-0.5 mL	0.4-0.5 mL	Not applicable	Not applicable	Not applicable	Not applicable	1 mL	1 mL	0.4-0.5 mL
Mean (median) DNA yield/ extraction <sup>1</sup>	12 ± 1.49 µg (12.56 µg)	4.40 ± 0.52 µg (2.06 µg)	4.29 ± 1.15 µg (2.63 µg)	0.29 ± 0.035 µg (0.297 µg)	0.374 ± 0.036 µg (0.345 µg)	Collection site dependent	1.22 ± 0.12 µg (0.86 µg)	1.22 ± 0.12 µg (0.86 µg)	--
Ambient temperature sample stability <sup>2</sup>	60 days	10 days (RNA) and 30 days (DNA)	30 days	30 days	30 days	30 days	21 days	21 days	7 days <sup>3</sup>

DNA Genotek products are compatible with a wide range of extraction kits.  
Please consult the specific product page or contact technical support (support@dnagenotek.com) for additional sample processing protocols and recommendations.

<sup>1</sup> Extraction from a 250 µL aliquot.

<sup>2</sup> Storage recommendations for samples collected with OMNIgene™ products from DNA Genotek™. DNA Genotek. PD-PR-01036

<sup>3</sup> Storage recommendations for samples collected with OMNImet™•GUT. DNA Genotek. PD-PR-00987

