

# Product change notification

**Products affected:**  **ORAc collect•Dx**



**Product SKU:** OCD-100 and OCD-100A

**Description:** ORAc collect•Dx

**Effective date of change:** May 2021

**Change description:** ORAc collect•Dx devices are currently packaged with an English only, folded instructions for use (IFU). The IFU is transitioning to a multi-language, multi-panel format.

## Product images:

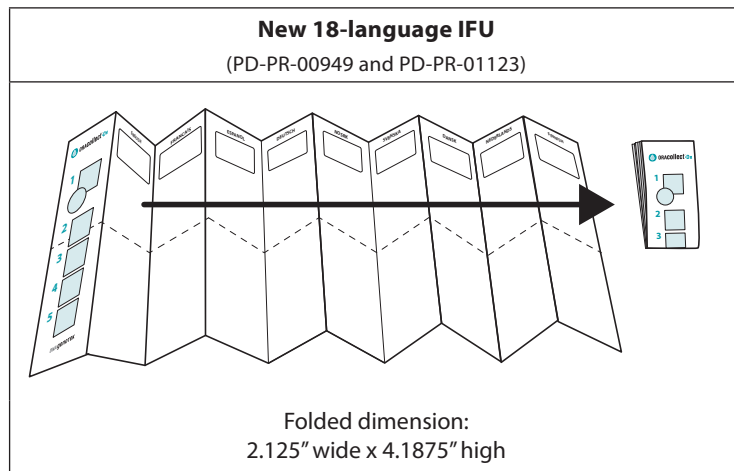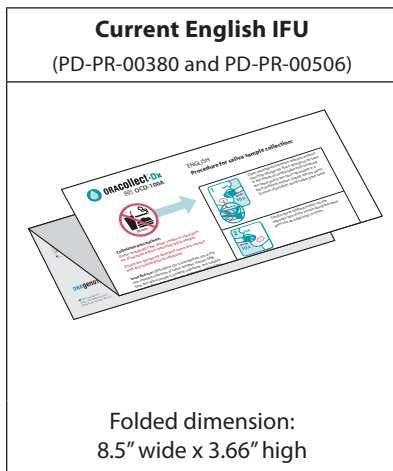

**Reason for change:** We are transitioning to a multi-language IFU to support customers who are using these products in the European Union and require compliance with the European Union Medical Device Regulation (EU MDR).

**Customer action:** No action is required.

Contact your DNA Genotek account manager or email [info@dnagenotek.com](mailto:info@dnagenotek.com) if you have any issues or concerns pertaining to this product change notification.